

## **IT-E151 Rack Mount Kit**

---

### **User 's Manual**

# **WARNING**

## **Safety Regulations**

To avoid electrical shock, do not open the cabinet. Refer servicing to qualified personnel only.

To avoid injuries always disconnect power, discharge circuits, and remove external voltage sources before touching components.

**KEEP AWAY FROM LIVE CIRCUITS.**

We cannot accept responsibility for any direct or indirect financial damage or loss of profit that might occur when using the power supply.

The instrument chassis and cover must be connected to an electrical ground.

## **Certification**

We certify that this product met its published specifications at time of shipment from the factory.

## **Warranty**

This hardware product is warranted against defects in material and workmanship for a period of ONE year from date of delivery. During the warranty period, our company will either repair or Replace product which is proved to be defective. For warranty service, with the exception of warranty options, this product must be returned to a service facility designated by our company. Customer shall prepay shipping charges by (and shall pay all duty and taxes) for products returned to our place for warranty service. Our company shall pay for return of products to customer.

## **Limitation of Warranty**

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by the Customer, Customer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation and maintenance.

## **Notice**

The information contained in this document is subject to change without notice.

# About IT-E151


IT-E151 rack mount kit is designed for using with IT6800, IT6900, IT6322, IT6120 , IT6400, IT6150 and IT6700 except IT6726 series power supply and IT8500 , IT8900, IT8811 and IT8812 series electronic load.

## Operation

First please remove the carrying handle and the two front hand feet.

### Action:

Grasp the handle and rotate it to a special position to let the arrow on the handle and the arrow on the front hand foot be in opposite directions. Fix up one side of the handle and pull another side outward, remove it from the front hand foot. And then remove the two front hand feet by a screwdriver.




the front hand foot

### Step for rack mounting a single instrument:


- ① Fix up the fitting on one side of instrument where the hand foot is by a bolt.
- ② Put the instrument into IT-E151 rack mount kit, fix up it together with the rack mount kit through the fitting.
- ③ Fix up the instrument with the rack mount kit from another side where the front hand foot is.



the fitting

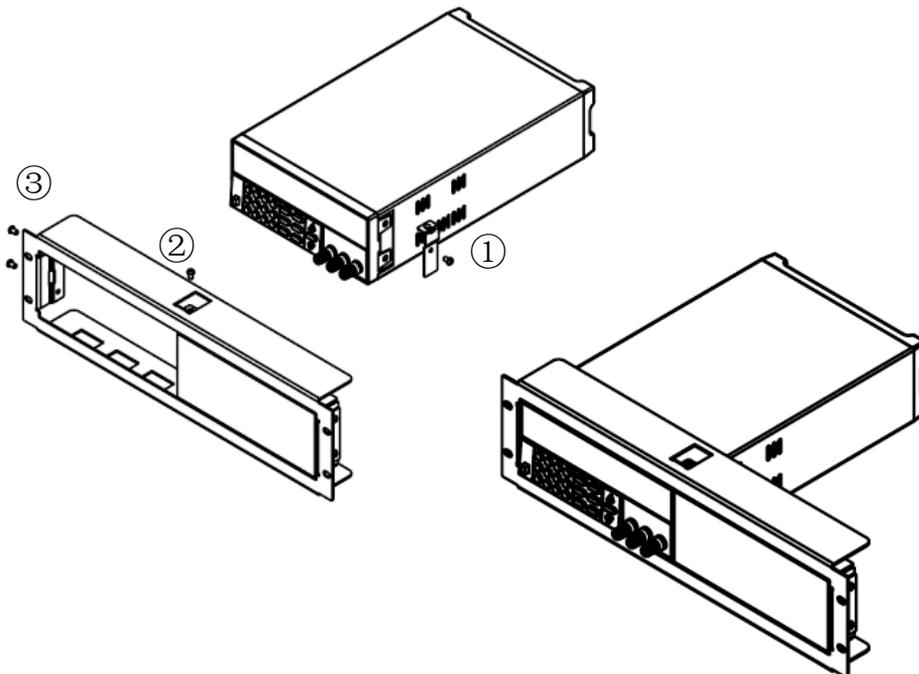


## Frontal view of rack mounting a single instrument

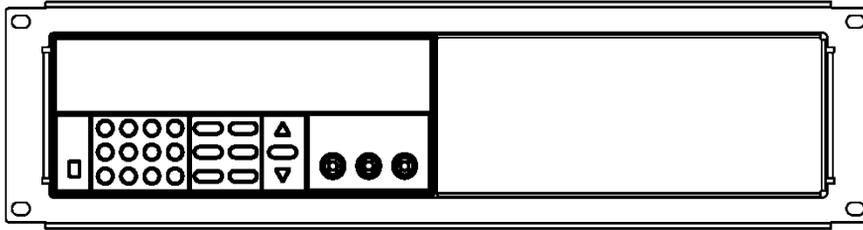


## Step for rack mounting two instruments:

- ① Remove the front cover panel on IT-E151 rack mount kit
- ② Fix up the fitting on one side of instrument A and B where the hand foot is by a bolt.
- ③ Put the instrument A into IT-E151 rack mount kit, fix up it together with the rack mount kit through the fitting.
- ④ Put the instrument B into IT-E151 rack mount kit, fix up it together with the rack mount kit through the fitting.
- ⑤ Fix up the two instrument with the rack mount kit from another side where the front hand foot is.

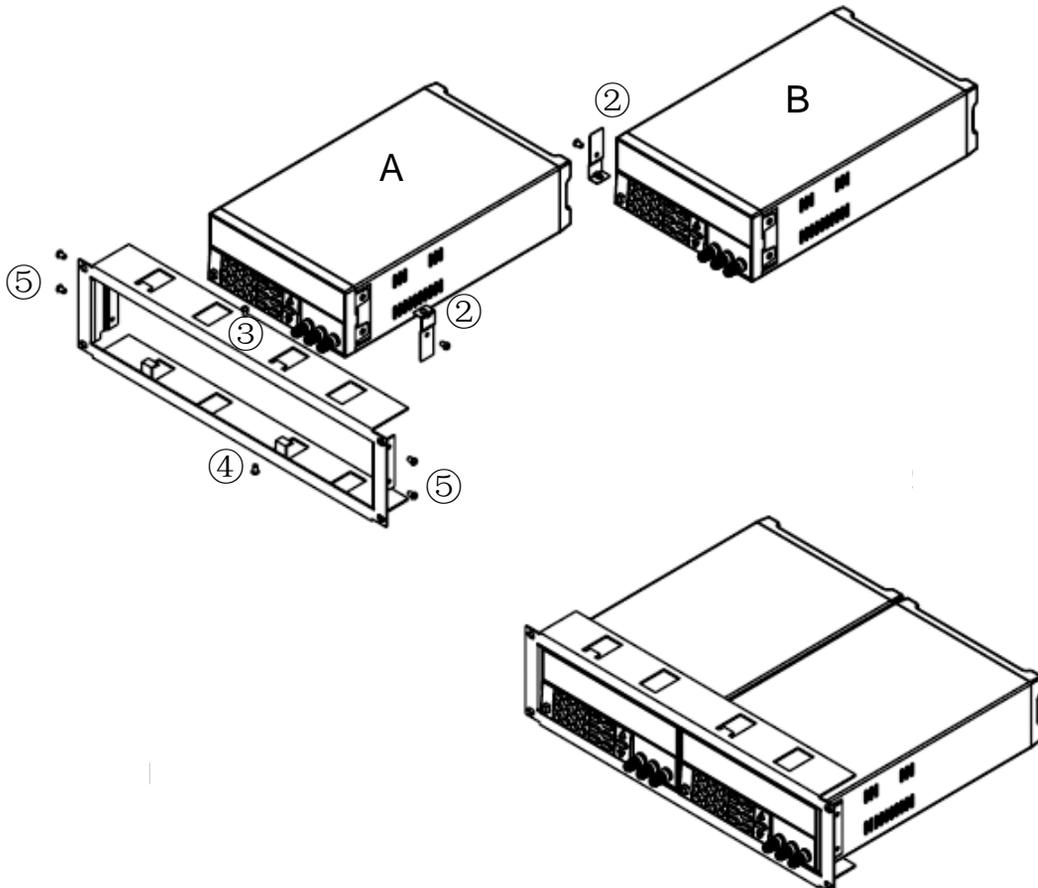


## Frontal view of rack mounting two instruments

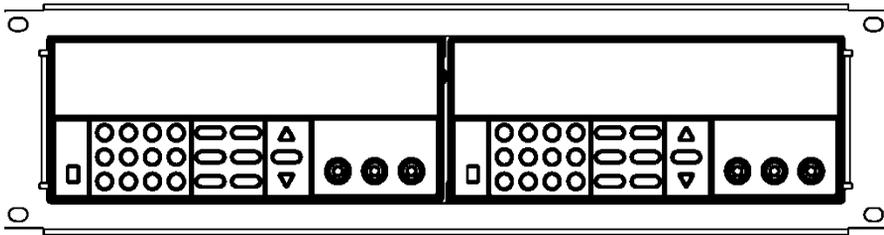


### Step for rack mounting the big instrument:


- ① Remove the two front hand foot and the foot on the bottom.
- ② Remove the front cover panel on IT-E151 rack mount kit.
- ③ Put the instrument into IT-E151 rack mount kit, and fix up it with the rack mount kit from two sides where the front hand foot is.




the front hand foot

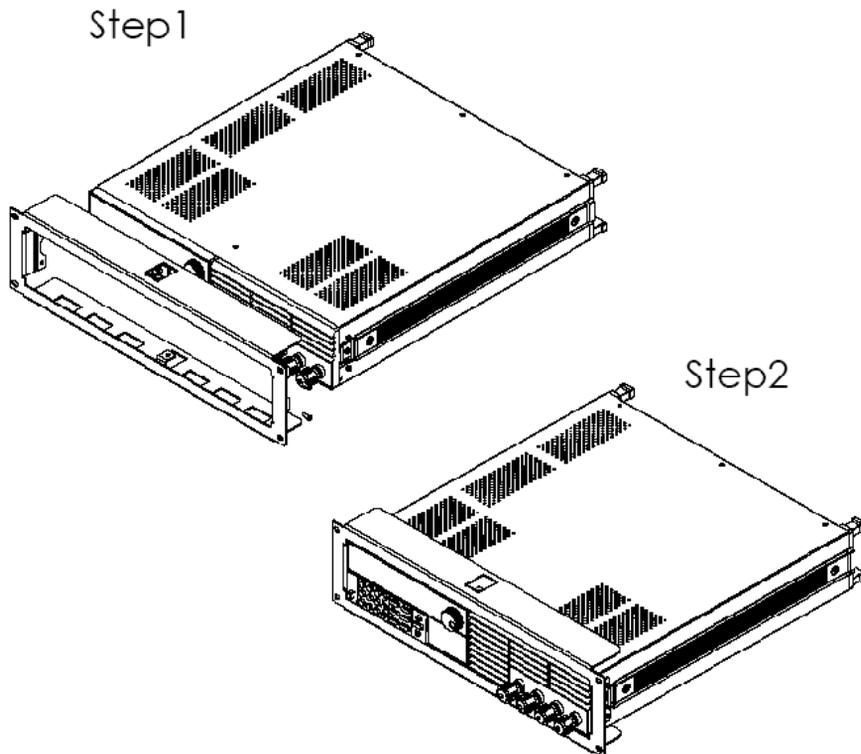

## Frontal view of rack mounting the big instrument

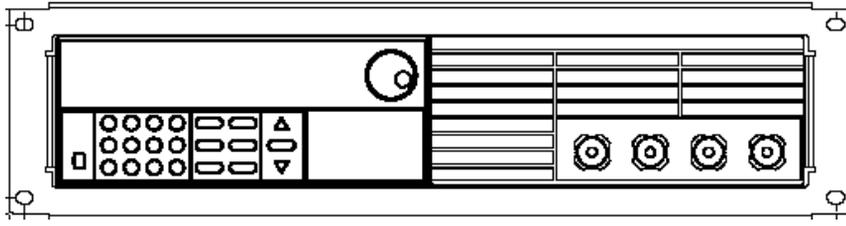

## Detailed Dimension Drawing

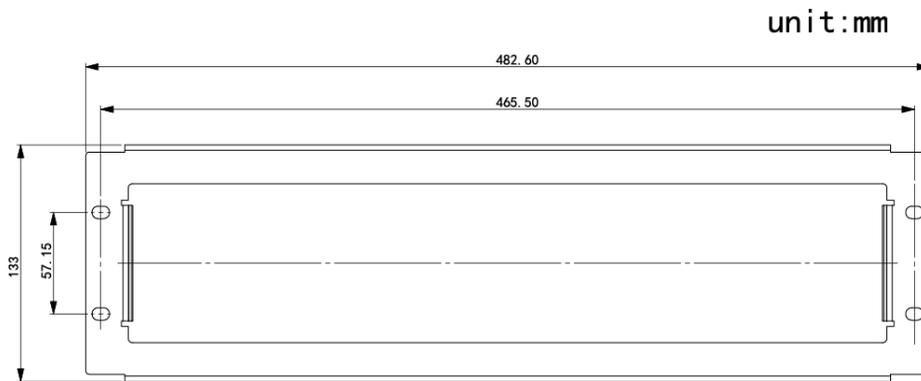



YOUR POWER TESTING SOLUTION



## Contact US

Thank you for purchasing ITECH products. If you have any doubt about this product, please contact us as follows.

1. Please refer to the CD-ROM of related user's manual in package.
2. Click [www.itechate.com](http://www.itechate.com) or scan the right two-dimensional code to visit the ITECH website.
3. Send E-mail to [fae@itech.sh](mailto:fae@itech.sh) or dial the service hot-line in China: 4006025000
4. Select the most convenient contact method for further consultancy.

